

# Alcotest 7110 Calibration Record

## Equipment

Alcotest 7110 MKIII-C  
Location: MONTCLAIR POLICE  
Serial No.: ARXA-0063  
Calibration File No.: 00832  
Calib. Date: 04/09/2021  
Calib. No.: 00033  
Certification File No.: 00816  
Cert. Date: 12/22/2020  
Cert. No.: 00027  
Linearity File No.: 00817  
Lin. Date: 12/22/2020  
Lin. No.: 00027  
Solution File No.: 00829  
Soln. Date: 03/17/2021  
Soln. No.: 00169  
Sequential File No.: 00832  
File Date: 04/09/2021


Calibrating Unit: WET  
Control Solution %: 0.100%  
Solution Control Lot: 19280  
Model No.: CU-34  
Serial No.: DDXC S3-0153  
Expires: 10/16/2021  
Bottle No.: 0722

## Coordinator

Last Name: ARROYO  
First Name: MARCOS  
MI: A.  
Signature: Sgt. Mr. 6291  
Badge No.: 6291  
Date: 04/09/2021

\*Black Key Temperature Probe Serial.....# DDHA P2-072 (M)

\*Digital NIST Temperature Measuring System Serial.....# 200 357 812 (M)

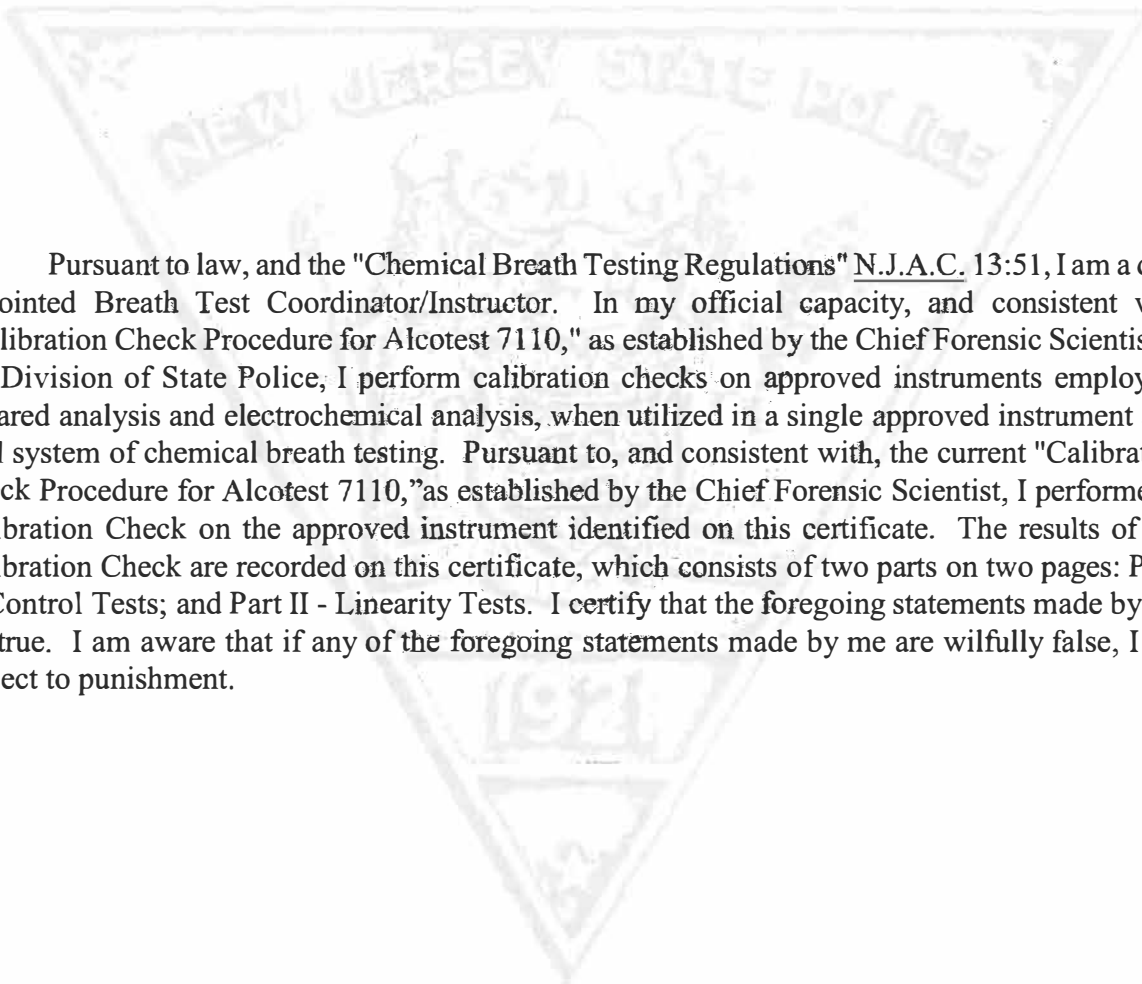

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0063  
Location: MONTCLAIR POLICE  
Calibration File No.: 00832 Calib. Date: 04/09/2021 Calib. No.: 00033  
Certification File No.: 00833 Cert. Date: 04/09/2021 Cert. No.: 00028  
Linearity File No.: 00817 Lin. Date: 12/22/2020 Lin. No.: 00027  
Solution File No.: 00829 Soln. Date: 03/17/2021 Soln. No.: 00169  
Sequential File No.: 00833 File Date: 04/09/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXC S3-0153  
Control Solution %: 0.100% Expires: 10/16/2021  
Solution Control Lot: 19280 Bottle No.: 0722

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 13:28D |                |                     |
| Control 1 EC      | 0.100% | 13:29D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.100% | 13:29D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:30D |                |                     |
| Control 2 EC      | 0.100% | 13:30D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 13:30D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:31D |                |                     |
| Control 3 EC      | 0.098% | 13:32D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.100% | 13:32D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:33D |                |                     |

All tests within acceptable tolerance.

### Coordinator

Last Name: ARROYO

First Name: MARCOS

MI: A.

Signature: Sgt. M. Arroyo

Badge No.: 6291

Date: 04/09/2021

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARXA-0063  
Location: MONTCLAIR POLICE  
Calibration File No.: 00832 Calib. Date: 04/09/2021 Calib. No.: 00033  
Certification File No.: 00833 Cert. Date: 04/09/2021 Cert. No.: 00028  
Linearity File No.: 00834 Lin. Date: 04/09/2021 Lin. No.: 00028  
Solution File No.: 00829 Soln. Date: 03/17/2021 Soln. No.: 00169  
Sequential File No.: 00834 File Date: 04/09/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0172  
Control Solution %: 0.040% Expires: 11/04/2021  
Solution Control Lot: 19310 Bottle No.: 1035

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0181  
Control Solution %: 0.080% Expires: 11/11/2021  
Solution Control Lot: 19320 Bottle No.: 0353

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0200  
Control Solution %: 0.160% Expires: 12/02/2021  
Solution Control Lot: 19360 Bottle No.: 0088

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 13:39D |                |                     |
| Control 1 EC      | 0.042% | 13:39D | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.039% | 13:39D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:41D |                |                     |
| Control 2 EC      | 0.041% | 13:41D | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.040% | 13:41D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:43D |                |                     |
| Control 3 EC      | 0.083% | 13:44D | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.079% | 13:44D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:45D |                |                     |
| Control 4 EC      | 0.081% | 13:46D | 34.0°C         | *** TEST PASSED *** |
| Control 4 IR      | 0.079% | 13:46D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:47D |                |                     |
| Control 5 EC      | 0.160% | 13:48D | 34.0°C         | *** TEST PASSED *** |
| Control 5 IR      | 0.157% | 13:48D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:50D |                |                     |
| Control 6 EC      | 0.154% | 13:51D | 34.0°C         | *** TEST PASSED *** |
| Control 6 IR      | 0.159% | 13:51D | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 13:52D |                |                     |

All tests within acceptable tolerance.

### Coordinator

Last Name: ARROYO

First Name: MARCOS

MI: A.

Signature: Sgt. M Arroyo

Badge No.: 6291

Date: 04/09/2021

# Calibrating Unit

## New Standard Solution Report

|                         |                       |              |            |
|-------------------------|-----------------------|--------------|------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C | Serial No.:  | ARXA-0063  |
| Location:               | MONTCLAIR POLICE      | Calib. Date: | 04/09/2021 |
| Calibration File No.:   | 00832                 | Calib. No.:  | 00033      |
| Certification File No.: | 00833                 | Cert. Date:  | 04/09/2021 |
| Linearity File No.:     | 00834                 | Lin. Date:   | 04/09/2021 |
| Solution File No.:      | 00835                 | Soln. Date:  | 04/09/2021 |
| Sequential File No.:    | 00835                 | File Date:   | 04/09/2021 |

|                       |        |            |       |             |              |
|-----------------------|--------|------------|-------|-------------|--------------|
| Calibrating Unit:     | WET    | Model No.: | CU-34 | Serial No.: | DDXC S3-0153 |
| Control Solution %:   | 0.100% |            |       | Expires:    | 03/30/2022   |
| Solution Control Lot: | 20180  |            |       | Bottle No.: | 1035         |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 15:02D        |                               |                           |
| Control 1 EC      | 0.102%         | 15:03D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.100%         | 15:03D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 15:04D        |                               |                           |
| Control 2 EC      | 0.101%         | 15:04D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.101%         | 15:04D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 15:05D        |                               |                           |
| Control 3 EC      | 0.101%         | 15:06D        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.099%         | 15:06D        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 15:06D        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDLA P3-0017 (M)

**Changed By:**

Last Name: ARROYO

First Name: MARCOS

MI: A.

Signature: \_\_\_\_\_

Sgt. Mr 6291

Badge No.: 6291

Date: 04/09/2021

**Alcotest 7110 MKIII-C Calibration  
NIST-Traceable Digital Thermometer Readings**

**Coordinator:**

Sgt. Marcos Arroyo  
Name

6291  
Badge No.

**Location:**

Mantoloking Police  
Agency

ARXA-0063  
Alcotest Serial No.

**Equipment:**

200 357812  
Digital NIST Temperature Measuring System Serial No.

| Simulator Solution Concentration | CU-34 Simulator Serial No. | Time Simulators Started to Heat | Time Temp. Reading Obtained | Temp. Reading on NIST Traceable Thermometer |
|----------------------------------|----------------------------|---------------------------------|-----------------------------|---|
| 0.04%                            | DDWES3-0172                | 12:05 <sub>D</sub>              | 13:10 <sub>D</sub>          | 34.0 <sup>o</sup> C                         |
| 0.08%                            | DDXDS3-0181                | 12:05 <sub>D</sub>              | 13:11 <sub>D</sub>          | 34.0 <sup>o</sup> C                         |
| 0.10%                            | DDXCS3-0153                | 12:05 <sub>D</sub>              | 13:12 <sub>D</sub>          | 34.0 <sup>o</sup> C                         |
| 0.16%                            | DDWES3-0200                | 12:05 <sub>D</sub>              | 13:13 <sub>D</sub>          | 34.0 <sup>o</sup> C                         |

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius  $\pm$  0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Sgt. M. Arroyo  
Coordinator's Signature

4/9/2021  
Date



## Alcotest 7110

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:                      Serial Number:

12-18-19                      ARXA-0063

Draeger, Inc.

*JS*, BS



**Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001**



**Cert. No.: 4000-11349766**

**Traceable® Certificate of Calibration for Digital Thermometer**

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

**Instrument Identification:**

Model: 61220-601, S/N: 200357812 Manufacturer: Control Company

**Standards/Equipment:**

| Description                  | Serial Number | Due Date    | NIST Traceable Reference |
|------------------------------|---------------|-------------|--------------------------|
| Thermistor Module            | A27129        | 04 Feb 2021 | 1000451212               |
| Temperature Calibration Bath | A42238        |             |                          |
| Temperature Calibration Bath | B01375        |             |                          |
| Temperature Probe            | 5394          | 21 Feb 2021 | C0220030                 |
| Temperature Calibration Bath | B16388        |             |                          |
| Temperature Probe            | 5267          | 21 Feb 2021 | C0220028                 |
| Temperature Calibration Bath | B3A444        |             |                          |
| Thermistor Module            | B96381        | 16 Jul 2020 | B9626028                 |
| Temperature Probe            | 5398          | 16 Jul 2020 | B9605083                 |
| Thermistor Module            | B96382        | 19 Aug 2020 | B9628006                 |
| Temperature Probe            | 5410          | 13 Sep 2020 | B9801031                 |

**Certificate Information:**

Technician: 420 Procedure: CAL-06 Cal Date: 15 Jun 2020 Cal Due Date: 15 Jun 2022  
 Test Conditions: 52.44%RH 23.46°C 1018mBar

**Calibration Data: (New Instrument)**

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min    | Max     | ±U     | TUR  |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|--------|------|
| °C      | N.A.    | N.A.     |        | 0.000   | 0.001   | Y      | -0.05  | 0.05    | 0.0087 | >4:1 |
| °C      | N.A.    | N.A.     |        | 25.001  | 25.001  | Y      | 24.951 | 25.051  | 0.0087 | >4:1 |
| °C      | N.A.    | N.A.     |        | 50.002  | 50.002  | Y      | 49.952 | 50.052  | 0.0087 | >4:1 |
| °C      | N.A.    | N.A.     |        | 100.003 | 100.004 | Y      | 99.953 | 100.053 | 0.0087 | >4:1 |

**This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.**

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement : (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ± U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

*Nicol Rodriguez*  
 Nicol Rodriguez, Quality Manager

*Marisa Elms*  
 Marisa Elms, Technical Manager

Note :

**Maintaining Accuracy:**

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598  
 Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com**

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
 Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.  
 International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349766

**Traceable® Certificate of Calibration for Digital Thermometer**

---

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

---

Issue Date : 15 Jun 2020

---

**CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598**  
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.  
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:      Certification Date:      Next Certification Due:

DDHHP2-072

6.3.20

6.3.21

Probe Value:

104

Draeger, Inc.

MAB

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

Model: ALCOTEST CU34

Model: MARK IIA

X-Cal 2000 (Alcosim)

Other: \_\_\_\_\_

Serial Number:

DDWES3-0172

Certification Date:

6.2.20

Technician:

MAB

Re-Certification Due Date:

6.2.21

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: \_\_\_\_\_

Serial Number:

DDXDS3-0181

Certification Date:

6-2-20

Technician:

MB

Re-Certification Due Date:

6-2-21

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

- Model: ALCOTEST CU34
- Model: MARK IIA
- X-Cal 2000 (Alcosim)
- Other: \_\_\_\_\_

Serial Number:

DDWES3-0200

Certification Date:

6-3-20

Technician:

MB

Re-Certification Due Date:

6-3-21

# Dräger Simulator

## CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to Calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

- Model: ALCOFEST-CU34
- Model: MARK IIA
- X-Cal-2000 (Alcosim)
- Other: \_\_\_\_\_

Serial Number:

DDXCS3-0153

Certification Date:

11.25.20

Technician:

OM

Re-Certification Due Date:

11.25.21

# Dräger

## Alcotest 7110 Temperature Probe

## CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDLAP3-0017

Certification Date:

11.25.20

Next Certification Due:

11.25.21

Probe Value:

103

Dräger, Inc. OM



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/25/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19280

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1212 to 0.1223 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 16, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/14/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19310

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 04, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 11/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19320

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0971 to 0.0985 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of November, 2019.

Notary.

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 12/11/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1956 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 02, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of December, 2019.
Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS
0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.

ANALYSIS DATE: 04/14/2020

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 20180

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1224 to 0.1233 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is March 30, 2022.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 16th day of April, 2020.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 60110522
My Commission Expires 01/13/2024



An Internationally Accredited Agency

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





ORIGINAL COURSE DATES

| DATE     | Refresher Course PLACE | INSTRUCTOR |
|----------|------------------------|------------|
| 1. _____ | _____                  | _____      |
| 2. _____ | _____                  | _____      |
| 3. _____ | _____                  | _____      |
| 4. _____ | _____                  | _____      |
| 5. _____ | _____                  | _____      |
| 6. _____ | _____                  | _____      |
| 7. _____ | _____                  | _____      |
| 8. _____ | _____                  | _____      |
| 9. _____ | _____                  | _____      |

S.P. 2938 (Rev. 07/07)

DEPARTMENT OF  
*Traffic and Public Safety*  
This is to certify that

MARCOS A. ARROYO  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE ALCOHOL TEST 7116 MKNIC  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 1st DAY OF May

TWO THOUSAND AND Nine

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE       | Refresher Course PLACE | INSTRUCTOR         |
|------------|------------------------|--------------------|
| 1. 8-13-08 | B.C.P.A.               | <i>[Signature]</i> |
| 2. 2/2/10  | SAKEVILLE PD           | <i>[Signature]</i> |
| 3. 2-7-12  | BERGEN C.P.A.          | <i>[Signature]</i> |
| 4. 9-2-14  | BERGEN C.P.A.          | <i>[Signature]</i> |
| 5. 6/30/16 | OLPA                   | <i>[Signature]</i> |
| 6. 12-4-18 | SAKEVILLE PD           | <i>[Signature]</i> |
| 7. 3/9/20  | BCPA                   | <i>[Signature]</i> |
| 8. _____   | _____                  | _____              |
| 9. _____   | _____                  | _____              |

S.P. 2938 (Rev. 12/04)

DEPARTMENT OF  
*Traffic and Public Safety*  
This is to certify that

MARCOS A. ARROYO JR.  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE ALCOHOL TEST 7116 MKNIC  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF February

TWO THOUSAND AND FIVE

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

| DATE        | Refresher Course PLACE | INSTRUCTOR         |
|-------------|------------------------|--------------------|
| 1. 10/10/06 | OLPA                   | <i>[Signature]</i> |
| 2. 9-5-08   | BLPP                   | <i>[Signature]</i> |
| 3. _____    | _____                  | _____              |
| 4. _____    | _____                  | _____              |
| 5. _____    | _____                  | _____              |
| 6. _____    | _____                  | _____              |
| 7. _____    | _____                  | _____              |
| 8. _____    | _____                  | _____              |
| 9. _____    | _____                  | _____              |

S.P. 2938 (Rev. 08/03)

DEPARTMENT OF  
*Traffic and Public Safety*  
This is to certify that

MARCOS A. ARROYO  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE ALCOHOL TEST 7116 MKNIC  
A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF October

TWO THOUSAND AND Four

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY